

1/5

FIG. 1



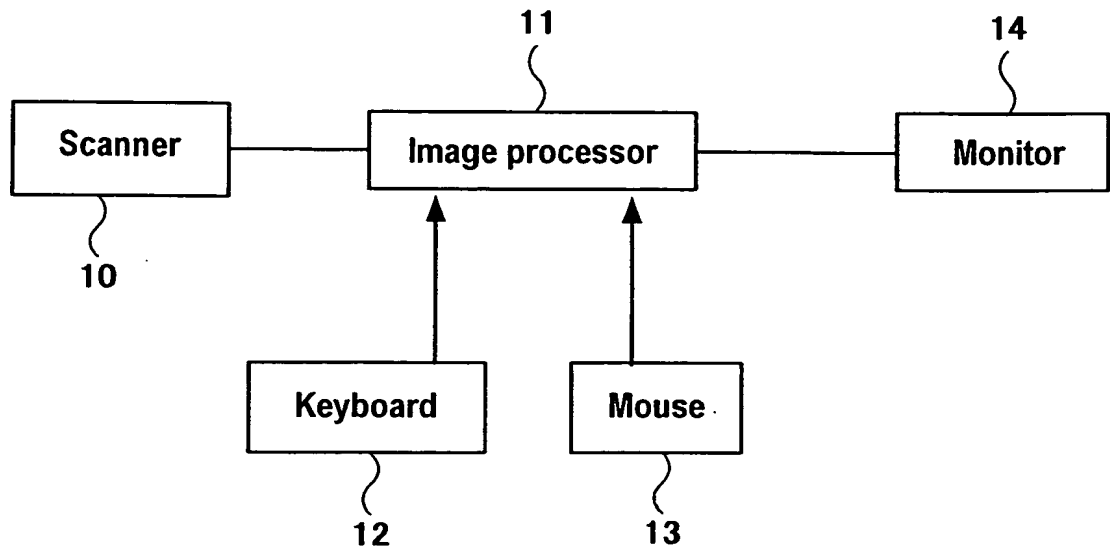


FIG. 3

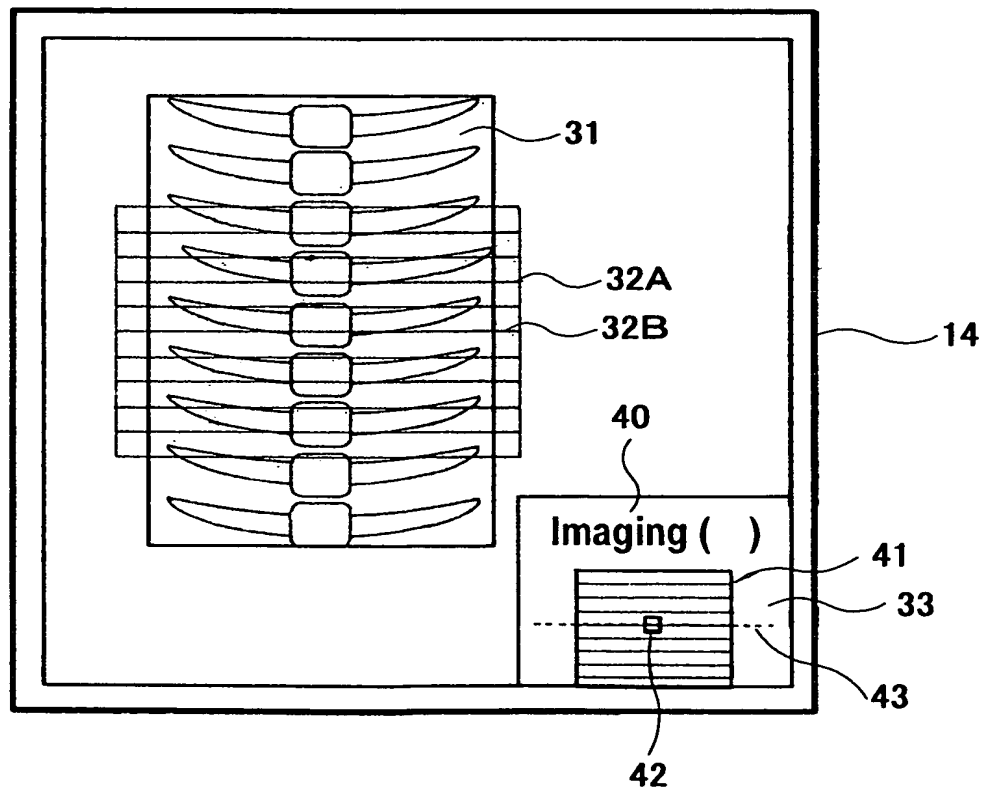

2/5

FIG. 2

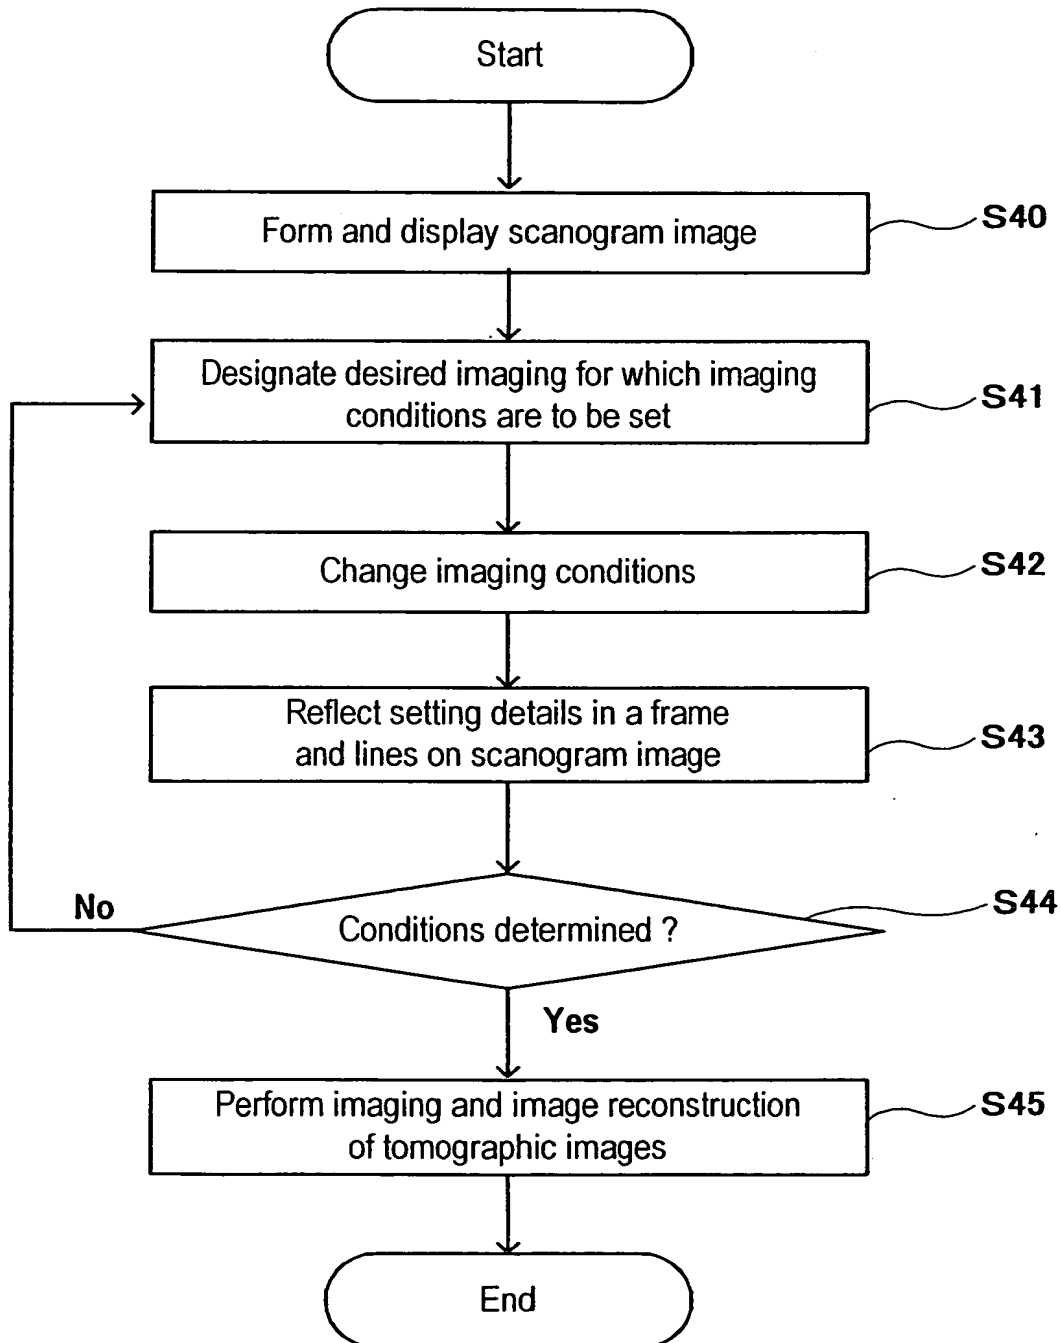

3/5

FIG. 4


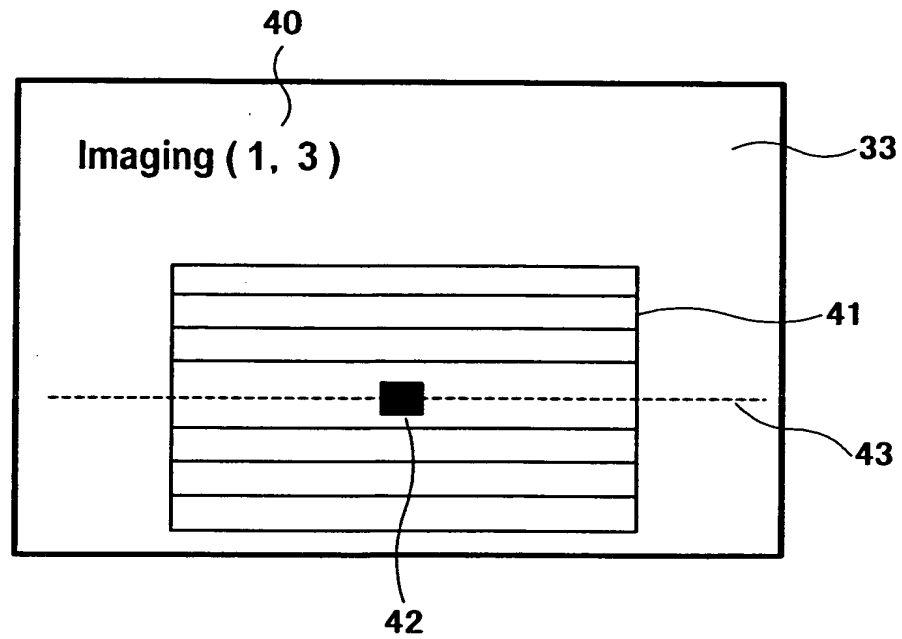


FIG. 5

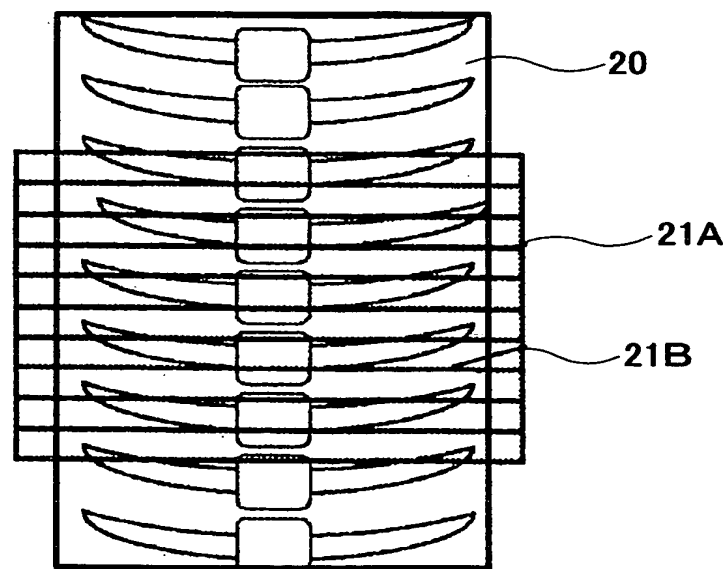

4/5

FIG. 6

100

SCAN

ONE
↓ TABLE
USUAL →
1/ 1

▲

▼

◀
END

Group name

Normal

Protocol name

(Y number of)Cervical vertebrae

▼

▲

XmA

5mm
Slice
thickness

YkV

▶
Preparations
for imaging

33

103

FIG. 7

101

No.	Group	Protocol
28	Normal	—
29	Normal	(X number of)Cervical vertebrae
30	Normal	(Y number of)Cervical vertebrae
31	Normal	—
32	Normal	—

No.	Input Code NV/D	Scan Number	Bed position (mm)	Gantry Angle	Total Scanning Time(s)
1	Normal	A	-2.0	0	1
2	Normal	A	-2.0	0	3
3	Normal	A	-2.0	0	1
4	Normal	A	-2.0	0	3
5	Normal	A	-2.0	0	1
6	Normal	A	-2.0	0	3
7	Normal	A	-2.0	0	1
8	Normal	A	-2.0	0	3
9	Normal	A	-2.0	0	1

Scan Range	

Protocol	Sequence
	END

102